Rev.04 01/2018

USE AND MAINTENANCE MANUAL

ERGOTHERAPY BOARD

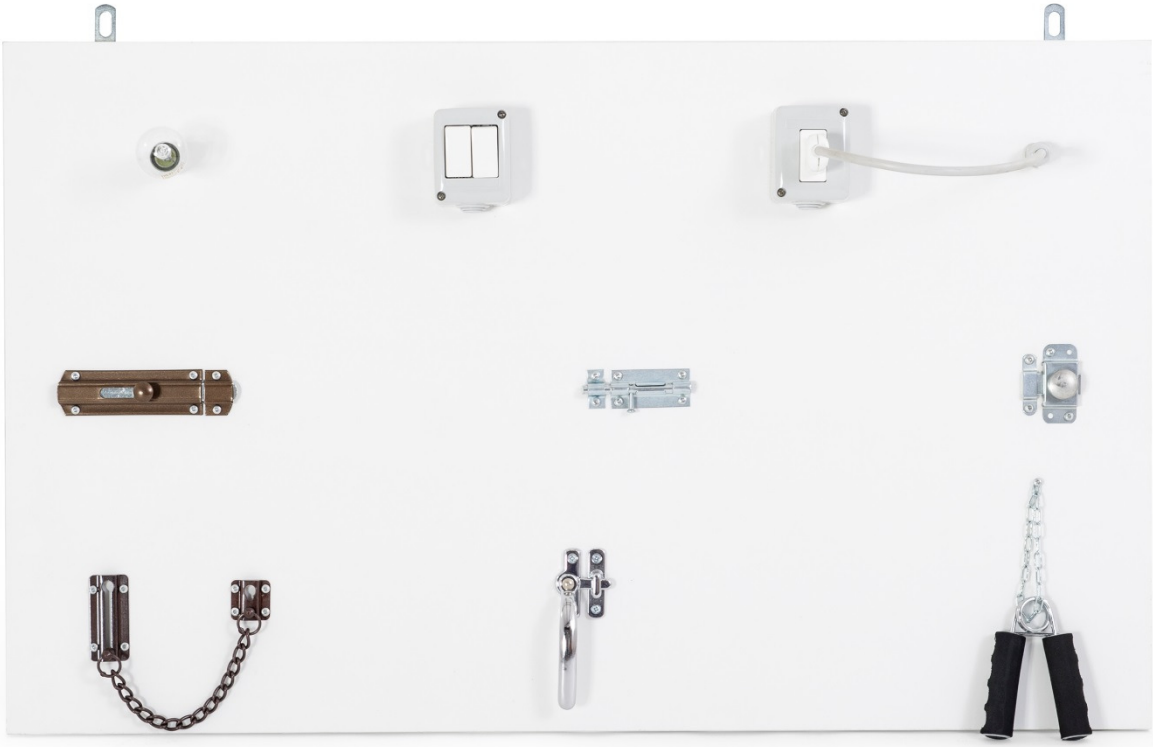

ERGOTHERAPY BOARD MODELS

Description	Code
Ergotherapy board 9 elements	135060

FISIOTECH SRL
Operating headquarters: Via Toniolo, 44/E-F - 31028 Vazzola (TV) - ITALY
Registered office: Via Valdoni, 19 - 31013 Cimavilla di Codognè (TV) - ITALY
Tel. +39 0438470342 - Fax +39 0438478762 - mail : info@fisiotech.com - pec : fisiotech@emailsec.it
VAT number IT 03765100262 - Rea TV 296956

Table of contents

INTRODUCTION	**p. 3**
SAFETY – WARRANTY	**p. 4**
DISPOSAL – DESCRIPTION	**p. 5**
ASSEMBLY INSTRUCTIONS – HOW TO – WARNINGS	**p. 6**
MAINTENANCE – CLEANING	**p. 7**
INSPECTION DATA SHEET	**p. 8**

INTRODUCTION

The purpose of this manual is to provide users and operators with the necessary information to use the shoulder wheel properly, autonomously, and safely.
This manual contains information on the technical features, operation, maintenance, spare parts and security of the ergotherapy board.
This manual must always be carried with the equipment and stored with care so that the readability is not compromised.
In case of transfer of use to a third party, this manual must be transferred as well, along with the other documents, as provided by Council Directive 93/42/EEC.

Intended use
Wall-mounted device with 9 elements simulating daily household activities. The elements are fixed to the board.
Device for the rehabilitation of subjects with functional limitations requiring rehabilitation of fingers, hand and wrist.

Manufacturer's details
FISIOTECH SRL
Operating headquarters: Via Toniolo, 44/E-F
31028 VAZZOLA (TV) - Italy
Tel. +39 0438 470342
Fax +39 0438 478762
info@fisiotech.com

Storing
The equipment does not require particular environmental conditions. It should be used in a closed environment with the following conditions: temperature 5℃ ÷ 40℃ – humidity 10% ÷ 80 %.

WARNING! Thoroughly read the manual before use.

FISIOTECH SRL refuses any responsibility and is not liable in case any damage to people and/or goods caused by the improper use of the ergotherapy board, by negligent or not-qualified staff or by non compliance with these instructions occurs.

SAFETY

WARNING!

Do not use the ergotherapy board:

- If you have not properly installed and adjusted the device
- If its use is counterindicated or causes severe discomfort to the patient
- If it has been tampered with or modified
- With an inappropriate configuration or if you suspect it may harm the patient
- The parts of the board may catch fire when exposed to an open flame
- Do not spill liquids on the metal parts of the equipment.

The user's psychological and physical suitability of use should be approved by a professional.

- Do not use the device for aims that differ from those listed in this manual.
- Do not use the device exposed to the weather
- Do not use the device if you did not fix it to the wall correctly
- Do not spill liquids on the equipment.
- The therapist should always supervise the patient during use.
- The manufacturer reserves the right to modify the product and this manual without notice in order to improve its features.

WARNING!

- Thoroughly follow this manual to use the product correctly.
- Keep the packaged product away from any source of heat. The packaging is made of cardboard.
- The lifespan of the equipment is linked to the wear of non-repairable and/or non-replaceable parts.
- Be careful to the moving parts, as they could cause injuries and the limbs may be caught in them.
- Be careful to children.
- Always check with your therapist and doctor before any rehabilitation therapy.

WARRANTY

The warranty of the ergotherapy board covers only the manufacturing defects for 24 months starting from the date of delivery. The warranty does not cover: consumables and items of normal wear such as: all 9 elements, breakdowns caused by any impact and/or fall, wrong or improper use, use by non qualified personnel. The warranty is void if the device has been tempered with. Warranty repairs are carried out at our operational headquarters and prior authorization. The products to be repaired under warranty must be shipped to the manufacturer freight prepaid and with the original packaging. A copy of the invoice and of the shipping document has to be sent along with a written request in order for the products to be repaired.

UNPACKING

	This symbol on a product means that it should not be thrown with regular waste, but disposed of following the laws on recycling/disposal in force in your country/region.

WARNING! The waste must be recycled. It should not be thrown with regular waste, but disposed of following the laws on recycling in force in your country/region.

DESCRIPTION
ERGOTHERAPY BOARD

Wall-mounted ergotherapy board with nine elements simulating daily household activities.

In particular the board mounts the following elements:

1. Light bulb
2. Switch
3. Plug
4. Bolt lock
5. Latch
6. Second bolt lock
7. Door chain
8. Window handle
9. Handgrips.

The ergotherapy board is sold without hardware.

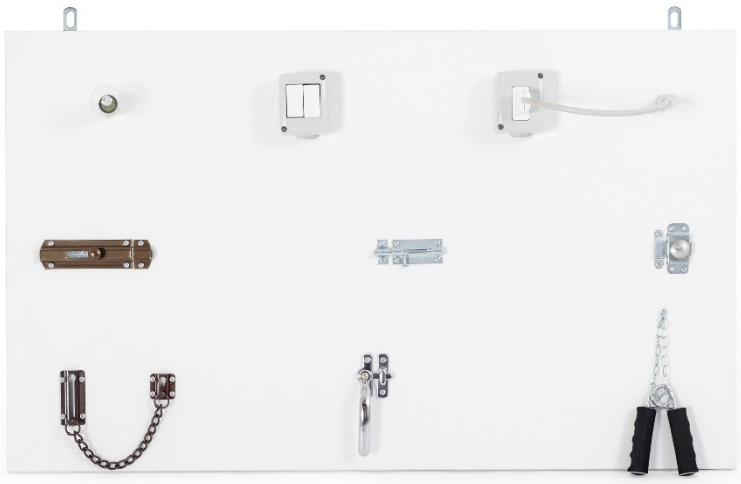

ASSEMBLY INSTRUCTIONS FOR THE ERGOTHERAPY BOARD

Before installing, verify the structural suitability of the environment and the appropriateness of the space available.

Take into account that installation requires technical qualifications, appropriate instruments and the help of at least one person.

Unpack and move the board with care. If you notice anomalies in the packaging and in the product do not install the equipment but inform the manufacturer immediately.

- Place the board on the wall and make sure it is centered and at the desired height.
- Draw the two points where you will pierce the wall with a pencil (in the center of the two eyelets)
- Pierce the wall with an equipment suitable to the type of wall.
- Insert the previously bought plugs according to the type of wall.
- Hang the ergotherapy board to the plugs with the eyelets

WARNINGS FOR USE

WARNING!

- Make sure that the ergotherapy board is correctly hung to the wall.
- Verify the function and state of all 9 elements.

WARNING

WARNING! The professional should never leave the patient unattended to prevent falls. The manufacturer is not liable for any damage to people and/or goods caused by negligent and/or not-qualified personnel.

MAINTENANCE

Maintenance must be carried out by a specialist, an electrician or someone who is familiar with the content of this manual.

Check the safety conditions of the device after any incident such as falls, violent impacts, spilling of liquids, etc. and any time you deem it necessary.

WARNING!

- In case of safety hazard, the device must be unplugged and is not to be used until safety is restored.

MAINTENANCE	WHAT TO DO
The ergotherapy board does not need a particular maintenance. We recommend you follow these steps:	Verify every three months, or after heavy usage, that it is well fixed to the wall Visual and functional inspection of all 9 elements.

CLEANING

Gently dust, and in case of light stains use a damp cloth or a neutral soap solution, rinsing with water. Let dry avoiding direct sunlight-

N.B. AVOID ALL ACID, ALCALINE AND SOLVENT PRODUCTS, SUCH AS ACETONE AND THINNERS.

FISIOTECH
TECNOLOGIE AL SERVIZIO DELLA SALUTE

INSPECTION RECORD SHEET

DEVICE MODEL / CODE:		INSTALLATION DATE	SERIAL No. .....
Inspection Date	**Maintenance**	**Name of the inspector**	**Signature**